
# GAMMA RADIATION NOT DEFLECTED IN A MAGNETIC FIELD

RAS 4.2

Required Kit:
DR991-1B Radioactivity, set

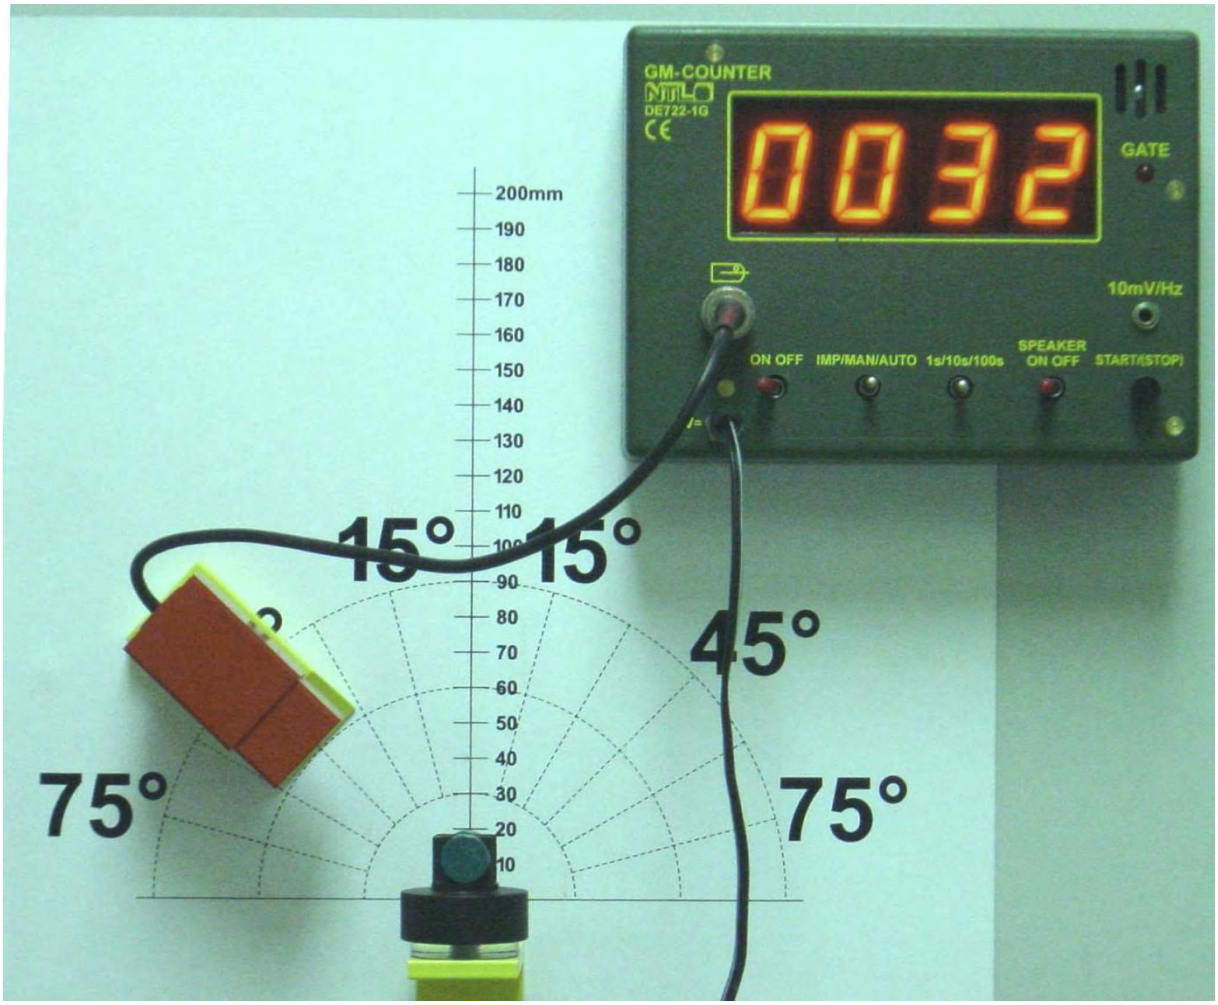


*Material:*

| Item Code | Qty | Description |
|---|---|---|
| DE407-1A | 1 | Magnets "neo", pair, button type, small |
| DE722-1G | 1 | Geiger-Mueller counter, "inno" |
| DR209-CO | 1 | Co-60 preparation (gamma radiation) |
| DR201-1R | 1 | Radioactive preparation mount, magnetic |
| DR213-1A | 1 | Adapter for deflection in radioactive substances |
| DR291-1Z | 1 | Geiger-Mueller tube on magnetic base |
| DR210-1F | 1 | Foil with scale, for radioactivity, magnetic (inno) |
| DR210-1P | 1 | Scale for radioactivity, metal (student) |

© Fruhmann GmbH, Austria